



EVERIC[®] plus

Pharmaceutical glass vial with barrier coating against leachables for sensitive formulations



- For highly sensitive drugs, leachables of the primary packaging into the drug product need to be minimized in order to protect their stability.
- The adsorption of proteins to the glass surface can result in conformational changes, denaturation, aggregation, and loss of effectiveness.
- EVERIC[®] plus vials have an ion barrier coating that can reduce adsorption and ensures low leachable levels for pharmaceutical products in the neutral and acidic pH ranges.
- Inner coating is applied using patented and proven plasma impulse chemical vapor deposition (PICVD) technology.
- An additional "release criterion" has been specifically developed.



SiO₂ layer applied via PICVD



Layer thickness of ~ 100–200 nm



Long-term layer stability



Coating bonds covalently to the glass substrate



Suitable for depyrogenation



Dense coating (i. e. non-porous)



Surface shows excellent barrier properties in reducing ion leaching: Na, Ca, B, Si, Al



Stable after washing process



Compliant with all current standards, such as Ph. Eur., USP, JP, and CP



Secured drug stability

Ion barrier provides stability for leachable sensitive drugs (e. g. radiopharmaceuticals and aluminum-sensitive drugs)



Reduced adsorption

For certain proteins, adsorption can be reduced thanks to a specialized inner surface*



Avoidance of pH-shift

Particularly relevant to WFI


* adsorption behavior needs to be tested case by case

Release test



1) Leaching


Autoclaving filled with 0.1 M HCl (pH 1 at start).



2) Determination of sodium via AAS

Certified release criterion for sodium (Na) – defined limit value.

Verifications: Avoidance of pH shift

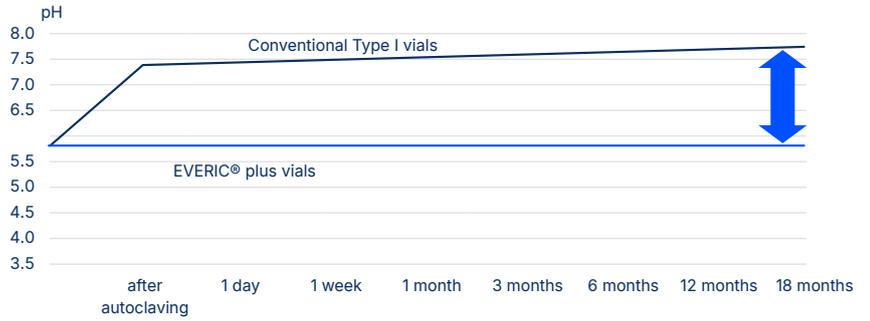


Method

10 ml vials, washed in accordance with ISO 4802. Autoclaving 1 h at 121°C. Storage at room temperature. Measurement of pH value prior to and after autoclaving (directly after, one day, one week, one/six/12/18 months).

Result

After autoclaving, conventional Type I vials show pH shifts from 5.5 up to 7.5. EVERIC® plus vials fully prevent pH shift.

Verifications: Secured drug stability

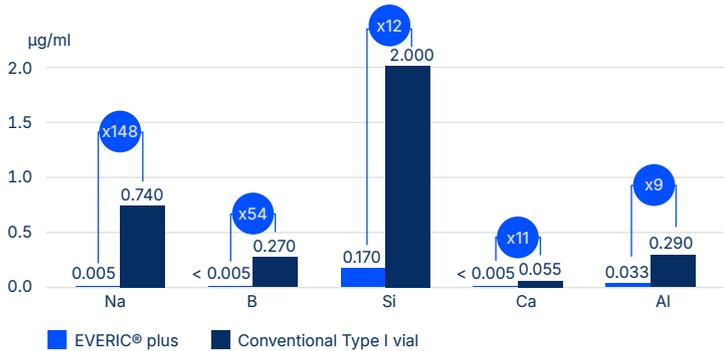


Method

10R vials, filled with purified water, 1 h autoclaving at 121°C. Leached ions in µg/ml by ICP-MS (ICP-OES for Si).

Result

The ion barrier is effective for all other elements of the glass matrix.

Verifications: Reduced adsorption

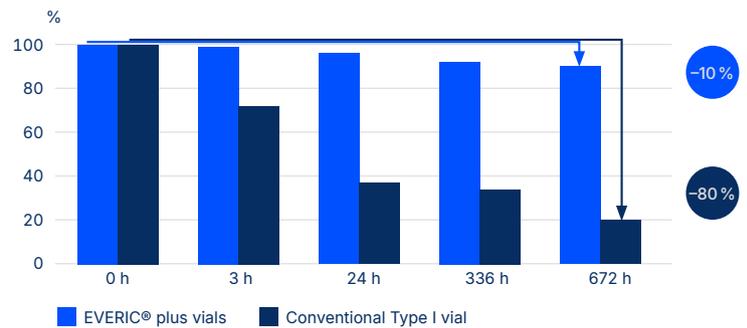

Method

Nicotinic acetylcholine receptor, concentration: 150 µg/ml, see: "A. Schrattenholz: Drug loss through adsorption of a nicotinic acetylcholine receptor in EVERIC® plus and standard vials".

Result

Tested protein shows less tendency to adsorb to EVERIC® plus vials.

General ordering information

Quality level	TopLine with additional release test											
Packaging	<ul style="list-style-type: none"> Tray with optional divider Pre-washed and pre-sterilized: adaptiQ® (tray, cup nest) 											
Palletizing	Standard Euro pallet (1200 x 800 mm) contains 15–27 layers of nine trays each											
Formats	2R	3R	4R	6R	8R	10R	15R	20R	25R	30R	50R	
Pieces per tray (non sterile)	344	344	344	186	186	154	154	95	95	95	40	

Many configurations are available in small quantities as "Fast Track Articles".

Visit our online shop or speak to your sales representative for more information.